
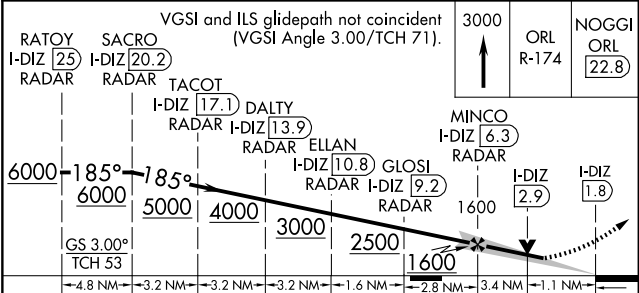


LOC/DME I-DIZ	APP CRS	Rwy Ldg
111.75	185°	10000
Chan 54 (Y)		TDZE 90
		Apt Elev 96

ILS or LOC RWY 17R
ORLANDO INTL (MCO)

RADAR required for procedure entry. DME or RADAR required.		ALSF-2	MISSED APPROACH: Climb to 3000 on ORL VORTAC R-174 to NOGGI/ ORL 22.8 DME and hold.
Simultaneous approach authorized. When using alternate missed approach, simultaneous approach NA. Bright lights on highway midway between Rwy 17L and Rwy 17R may be mistaken for runway lights.			

D-ATIS	ORLANDO APP CON	ORLANDO TOWER	GND CON
121.25	124.8 307.0	118.45 253.5 (17L/35R, 17R/35L) 124.3 253.5 (18L/36R, 18R/36L)	126.4 (E) 121.8 (W)

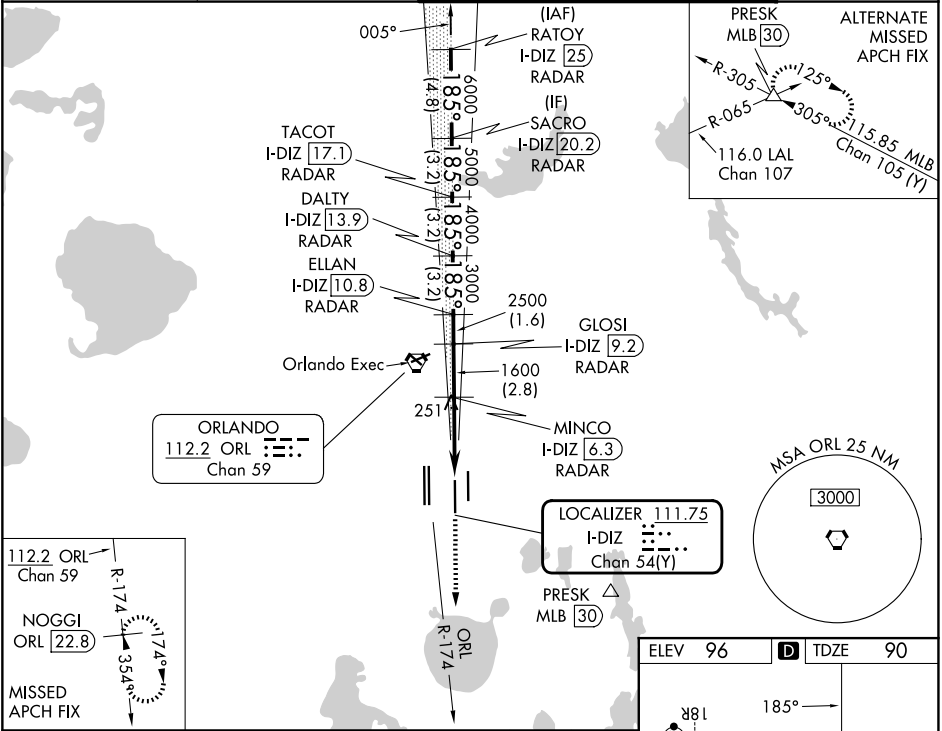

CATEGORY	A	B	C	D
S-ILS 17R	290/18 200 (200-½)			
S-LOC 17R	520/24 430 (500-½)		520/40 430 (500-¾)	
CIRCLING	740-1 644 (700-1)		740-1¾ 644 (700-1¾)	740-2 644 (700-2)

